

Operations Manual

Item: C1008

V1.0

myFUGE™ Mini



Introduction:

Thank you for purchasing the **MyFuge™** Mini Centrifuge. Please read this manual thoroughly prior to operating the instrument.

The **MyFuge** Mini Centrifuge is designed for low speed applications and quick spin downs of microcentrifuge tubes (0.2ml - 2.0ml) and for eight position PCR strips.

Specifications:

Speed: 6000 rpm / 2000xg
Capacity: 8 x 1.5/2.0ml
32 x 0.2ml or 4 x PCR strips
Dimensions: 5.7 (W) x 6.9 (D) x 4.5 (H) in.
14.5 (W) x 17.8 (D) x 11.4(H) cm
Electrical: 120V to 240V, 50-60 Hz, 50W
Max. Radius: 4.9cm

Installation:

Place the **MyFuge** mini-centrifuge on a flat and level surface nearby an electrical outlet. It should not be near a heat source or in direct sunlight.

Rotor Exchange:

The **MyFuge** mini-centrifuge includes a second rotor that is designed for holding PCR tubes (0.2ml) and PCR strips (8 position). The rotor is conveniently stored in a compartment on the bottom of the centrifuge. To access this rotor, turn the machine upside down and remove it from the compartment.


- Removing the Rotor from the motor shaft:

The new **Clik-n-Lok™** rotor attachment system allows for instant exchange of rotors. To remove a rotor, simply pull it upwards, off the shaft. (NO TOOL IS REQUIRED.)

- Attaching the Rotor to the motor shaft:

Place the rotor on the motor shaft and press down until the rotor comes to a stop. The rotor is now secured. (NOT TOOL IS REQUIRED)

Operation:


- Attach the power cord and place the power switch into the "on" position.
 - Open the lid and load your samples into the rotor. Always ensure a balanced load (Please see the following section, **Loading the Rotor**, for details.)
 - Close the lid, the rotor quickly accelerates to the maximum speed of 6200 rpm.
 - When the desired run time is completed, push on the lid button to open the lid, the rotor quickly brakes to a stop and the samples can be retrieved.
-  NEVER Attempt: to remove samples until the rotor has come to a complete stop.

Loading the Rotor:


To ensure safe operation and long life of the instrument, samples must always be loaded into the rotor in a balanced fashion.

Tubes and strips must always be loaded symmetrically across from one another and contain the same volume of liquid. See below:

Examples of properly balanced rotors:

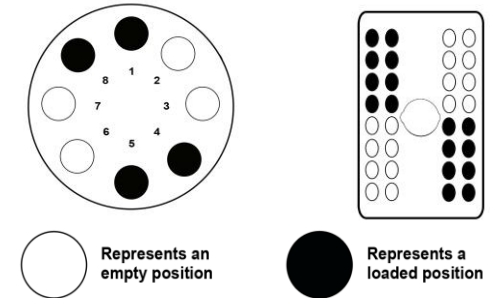

Examples of improperly balanced rotors:

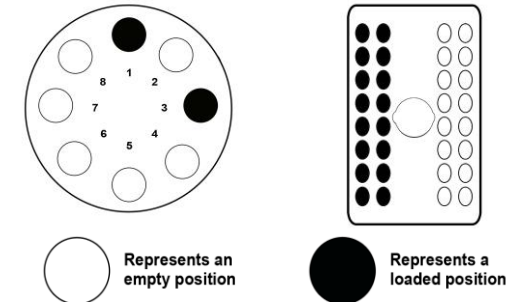

Cleaning and Maintenance:

The centrifuge rotors can be removed for cleaning. Once removed, the rotors can be cleaned with isopropyl alcohol or can be sterilized in an autoclave at 121°C for 20 minutes.

Service and Contact:

In the event that service or technical support is required, please contact **Benchmark** by phone at **1-908-769-5555**